

Research

*Corresponding author

Lei Lei

Department of Otolaryngology Head and Neck Surgery
Chinese PLA General Hospital
28 Fuxing Road
Beijing 100853, China
E-mail: wislei301@163.com

Volume 1 : Issue 1

Article Ref. #: 1000OTLOJ1106

Article History

Received: September 5th, 2015

Accepted: November 23rd, 2015

Published: November 25th, 2015

Citation

Lei L, Li J, Liu M, Hu X, Zhou Y. Shape from shading and optical flow used for 3-dimensional reconstruction of endoscope image. *Otolaryngol Open J.* 2015; 1(1): 20-23. doi: [10.17140/OTLOJ-1-106](http://dx.doi.org/10.17140/OTLOJ-1-106)

Copyright

©2015 Lei L. This is an open access article distributed under the Creative Commons Attribution 4.0 International License (CC BY 4.0), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Shape from Shading and Optical Flow used for 3-Dimensional Reconstruction of Endoscope Image

Lei Lei^{1*}, Jianhui Li^{1*}, Meiqing Liu², Xiaoming Hu² and Ya Zhou²

**These authors contributed equally*

¹Department of Otolaryngology Head and Neck Surgery, Chinese PLA General Hospital, 28 Fuxing Road, Beijing 100853, China

²School of Optoelectronics, Beijing Institute of Technology, 5 Zhongguancun Road, Beijing 100081, China

ABSTRACT

Recent year's endoscopy is widely used in computer assisted surgeries. Three-Dimensional (3D) reconstruction has been presented due to the lack of depth information from endoscope images. One of the fundamental approaches in the domain of computer vision is Shape From Shading (SFS). This algorithm was proposed to obtain the shape of an object from a single intensity image. Because of the severe conditions are required in shape from shading to reconstruct 3D surface. The photometric calibration is proposed from the view of image processing. The calibration is important for illumination-based visualization techniques such as shape-from-shading. The result showed that the stability of surface reconstruction is improved when the photometric calibration is used before shape from shading. But the surface reconstruction from Shape From Shading (SFS) is the relative variation in the gray gradient field. So, the change from relative variation to absolute variation is necessary when the actual size of surroundings have to be known. Then the optical flow is introduced to solve this change in my paper. The optical tracker is also used in this system to capture the pose of endoscopy.

KEYWORDS: Photometric calibration; 3D reconstruction; Shape from shading; Optical flow.

ABBREVIATIONS: 3D: Three-Dimensional; SFS : Shape From Shading; SIFT: Scale Invariant Feature Transform; PDE: Partial Differential Equations.

INTRODUCTION

3D reconstruction from endoscope image is a boomed technology in minimally invasive surgery, the lack of depth from endoscope image push the development of diverse technology in 3D reconstruction. The reconstruction of endoscopic sequence images¹ is being frequently studied during the past years. The feature matching between sequence images is important for the subsequent reconstruction. Scale Invariant Feature Transform (SIFT) is wildly used in image matching but suffered from low matching pairs when employed in endoscope image. In this paper, the Shape From Shading (SFS) is implemented to 3D reconstruction due to its advantage. The surface is reconstructed from only a single image when the SFS is used. Every pixel in image is used for reconstruction compared with the extracted feature points.

SFS is one of the key technologies for three-dimensional reconstruction in computer vision. The principle is to use the change of single image gray to restore the relative height or the normal vector of surface in each point.² SFS technology was first developed by MIT's Horn³ to solve the reconstruction of the lunar surface. He considered SFS problem as the inverse of the imaging process. The information of image gray is closely related with the intensity of surface reflection. Thus, the surface brightness can be changed to obtain the height information.

A few of recent works applied shape from shading to endoscopic images based on photometric calibration.⁴ However, in order to reconstruct an accurate shape from endoscopic images, the knowledge of light sources is necessary and important. The camera response function, light source intensity and light spatial distribution function are important when shape from shading method is used for the reconstruction. The gray card is produced by myself in this paper, which contains eighty percent to twenty percent gray. It can be regarded as the medium to calibrate the relationship between light source intensity and camera response function. When this relationship is illustrated with curve diagram, we can obtain the inverse of image intensity to compensate the original image.

In our work, an implemented photometric calibration is proposed which still performs well in synthetic image and real image. More detailed descriptions and experimental results of this method will be presented in Material and Methods. Finally, the conclusions are drawn in Discussion.

MATERIAL AND METHODS

The Construction of Non-Lambertian Reflection Model

The image irradiance equation based on the Oren-Nayar model⁵ is widely used in shape from shading and can be expressed as follow formulas.

$$I(x, y) = R(p, q) = \frac{A}{\sqrt{1+|\nabla z|^2}} + \frac{B|\nabla z|^2}{1+|\nabla z|^2} \quad (1)$$

Generally speaking, the radiation source toward the radiation intensity is different in all directions, having directionality. The object with that character is called Lambert reflector. And the light intensity is defined in the formula above. If the camera coordinate system is set as reference system, and the height of object surface is set as $z(x, y)$, so the object surface normal vector can be represented by a normal vector of the surface at various points $n=(n_1, n_2, n_3)$. $p = \partial z / \partial x$, $q = \partial z / \partial y$, $p = -n_1/n_3$, $q = -n_2/n_3$.

The Numerical Algorithm to Solve the PDE Equation

The SFS problem (1) can be formulated as the following Eikonal PDE:

$$|\nabla z(x, y)| = \sqrt{f^2 - 1} \quad \forall x \in \Omega$$

$$z(x, y) = \varphi(x, y) \quad \forall x \in \partial\Omega \quad (2)$$

A numerical algorithm based on the high-order Godunov fast sweeping scheme^{5,6} is proposed to solve the Eikonal

Partial Differential Equations (PDE) equation.

The Model of the Gray Card

The gray card is produced with the same radiance, which contains eighty percent to twenty percent gray. It can be regarded as the medium to calibrate the relationship between light source intensity and camera response function Figure 1.



Figure 1: The model of the gray card.

The Result of Experiment

When we get the curved diagram in Figure 2, we can obtain the inverse of image intensity to compensate the original image and the result is showed in Figure 3. In order to demonstrate the validity of this photometric calibration, the reconstruction implemented in synthetic and real image and the result shown in Figures 4 and 5. The action of the experiment is inspired by the model in paper.⁷

The curved diagram between camera response and image intensity.

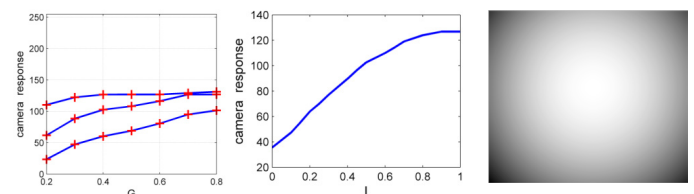


Figure 2: Left is the relationship between camera response and gray level (7 levels in my paper). The middle is relationship between camera response and image intensity. The right is the cosine term $\frac{n \cdot l}{r}$.

The Pseudo-color indicates the distribution of image intensity before and after calibration

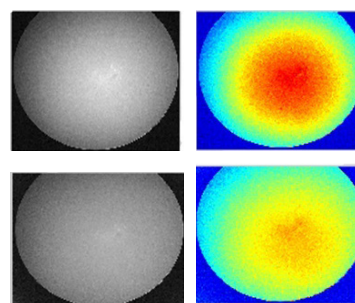


Figure 3: The upper set is indicating before calibration and the under set is indicating after calibration.

Synthetic image

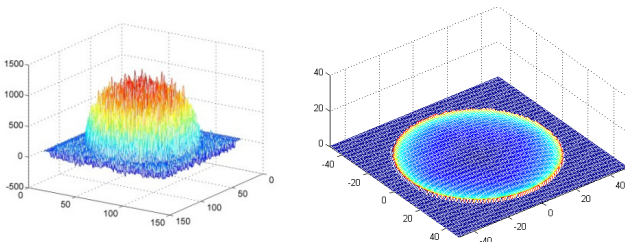


Figure 4: The left is the reconstruction of the synthetic sphere and the right is the error between ground truth and our reconstruction.

Real image

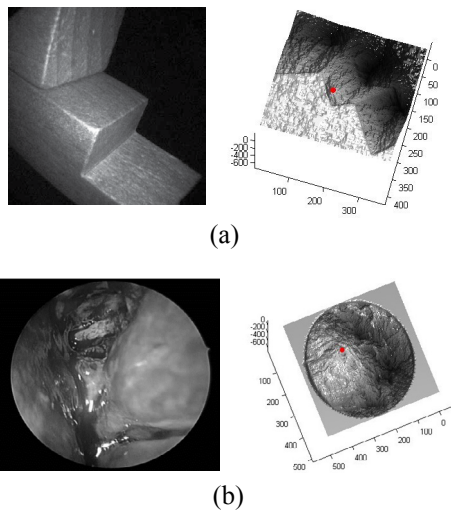


Figure 5: The real image reconstruction. Left is the original image and right is the corresponding reconstruction result in set of (a) and (b).

DISCUSSION

Because 3D reconstruction help doctors diagnose, so choose suitable endoscope under the environment of 3D reconstruction method is particularly important. During the project investigation and experiment analysis shows that although the contrast method has its unique advantages, but also has disadvantages:¹ To restore the depth of the surface is not absolute information, assuming assisted by endoscope can use external tracking equipment movement information, and then derive the depth of the surface information according to the relationship between image and object. But in the process of actual implementation need complex experimental system and equipment.² Although a single image can be restored to form, but general surgery are taken in the process of video images. So that by extending the way of the contrast method combining reconstruction of different gray gradient information, we can get endoscopic coordinates of 3D tissues and organs.

According to the algorithm of defect group we put forward the solution. If we want to reconstruct the 3D surface shape; we should transit it to the world coordinate system and get endoscopic pose information. Although optical tracker can

locate endoscopic posture, but due to the lack of trace markers and the transformation of the relationship between endoscopic, so it is difficult to transfer 3D surface shape to world coordinates. Provide extended way for doctors under the endoscopic view of tissues and organs of the three-dimensional topography, can be a good guide for doctor's surgery.

CONCLUSIONS

The small error in synthetic image demonstrates the validity of photometric calibration. The next mission is introducing the optical flow make the change from relative variation to absolute variation.

CONFLICTS OF INTEREST

The authors declare that they have no conflicts of interest.

ACKNOWLEDGEMENTS

The study was supported by The National Youth Nature Foundation (30900385), The People's Liberation Army General Hospital Clinical Scientific Research Foundation (2012FC-TSYS-3048).

The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.

REFERENCES

1. Du P, Zhou Y, Hu X. Improved SIFT matching algorithm for 3D reconstruction from endoscopic images. *ACM-SIGGRPH-VRCAI*. 2011; 12(1): 4-16.
2. Okatani T, Deguchi K. Shape reconstruction from an endoscope image by shape from shading technique for a point light source at the projection center. *Computer Vision and Image Understanding*. 1997; 66(2): 119-131. doi: [10.1006/cviu.1997.0613](https://doi.org/10.1006/cviu.1997.0613)
3. Horn BKP, Brooks MJ. The variational approach to shape from shading. *Computer Vision, Graphics, and Image Processing*. 1986; 33(2): 174-208.
4. Wu C, Jaramaz B, Narasimhan SG. A full geometric and photometric calibration method for oblique-viewing endoscope[J]. *Comput Aided Surgery*. 2010; 15(1-3): 19-31. doi: [10.3109/10929081003718758](https://doi.org/10.3109/10929081003718758)
5. Wang G, Liu S, Han J, Zhang X. A novel shape from shading algorithm for non-lambertian surfaces. *Measuring technology and mechatronics automation (ICMTMA), 2011 Third International Conference on Shanghai*. 2011; 1: 222-225.
6. Durou J-D, Falcone M, Sagona M. Numerical methods for shape from shading: a new survey with benchmarks. *Computer Vision and Image Understanding*. 2008; 109(1): 22-43. doi:

[10.1016/j.cviu.2007.09.003](https://doi.org/10.1016/j.cviu.2007.09.003)

7. Litvinov A, Schechner YY. Addressing radiometric nonidealities: a unified framework. *Proceedings of the 2005 IEEE Computer Society Conference on Computer Vision and Pattern Recognition(CVPR'05)*. 2005; 2: 52-59. doi: [10.1109/CVPR.2005.64](https://doi.org/10.1109/CVPR.2005.64)